OIPE JC139
MAR 15 2004
PATENT & TRADEMARK OFFICE

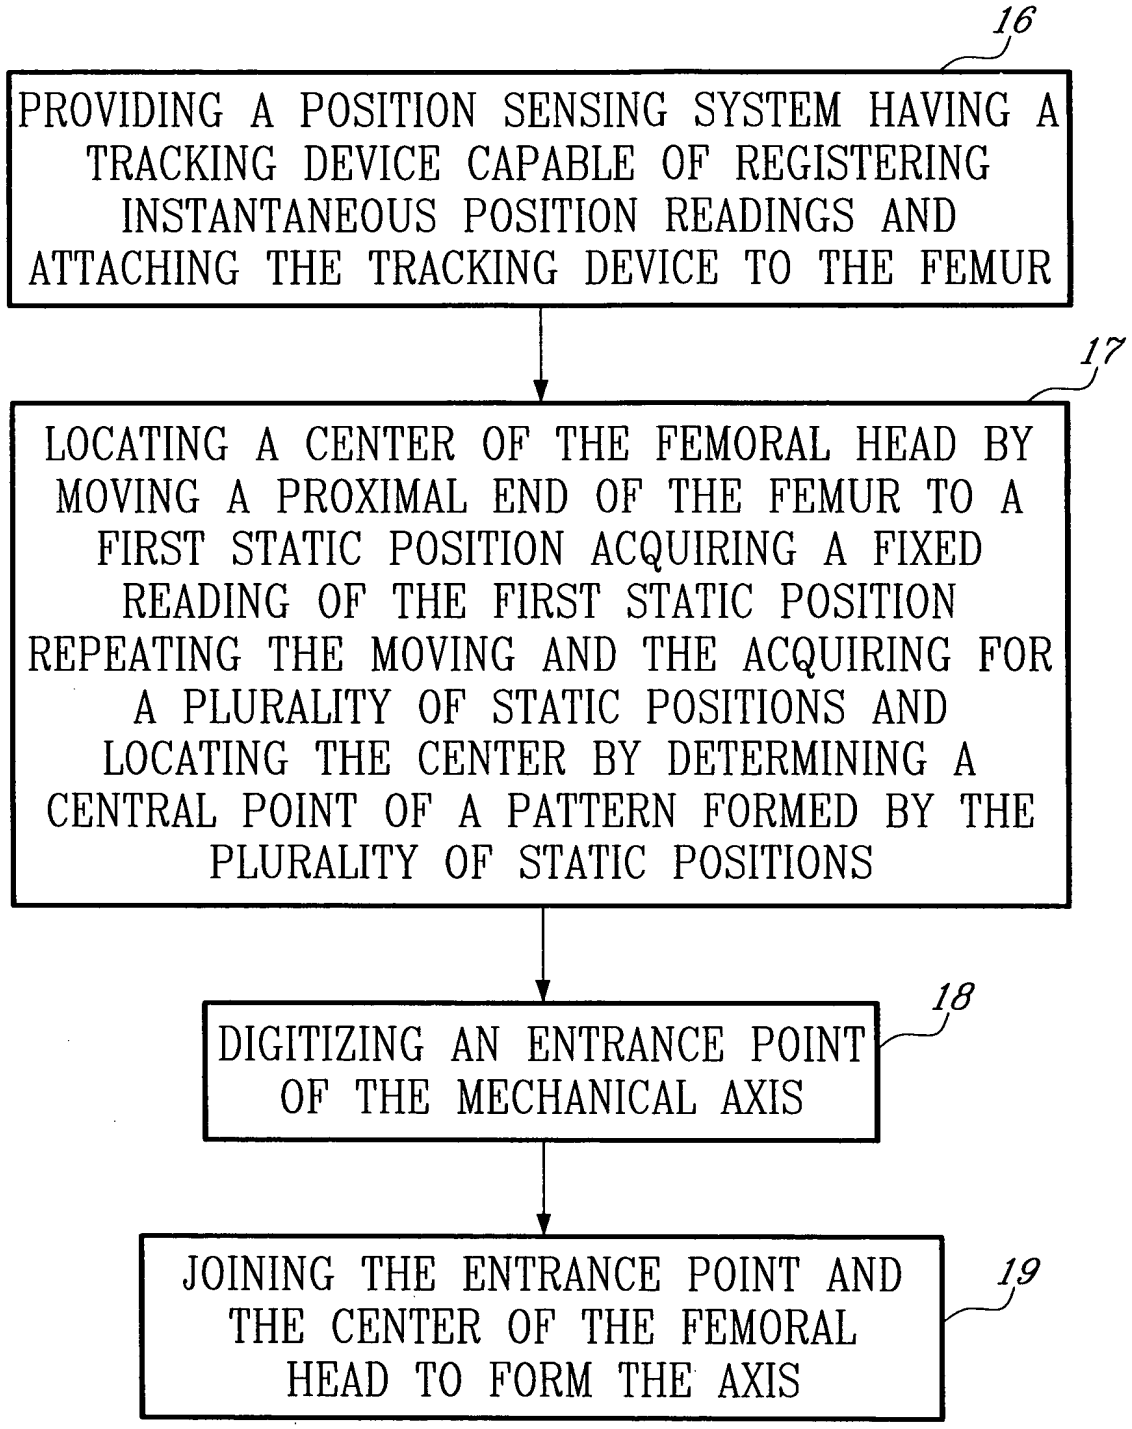

Fig. 1

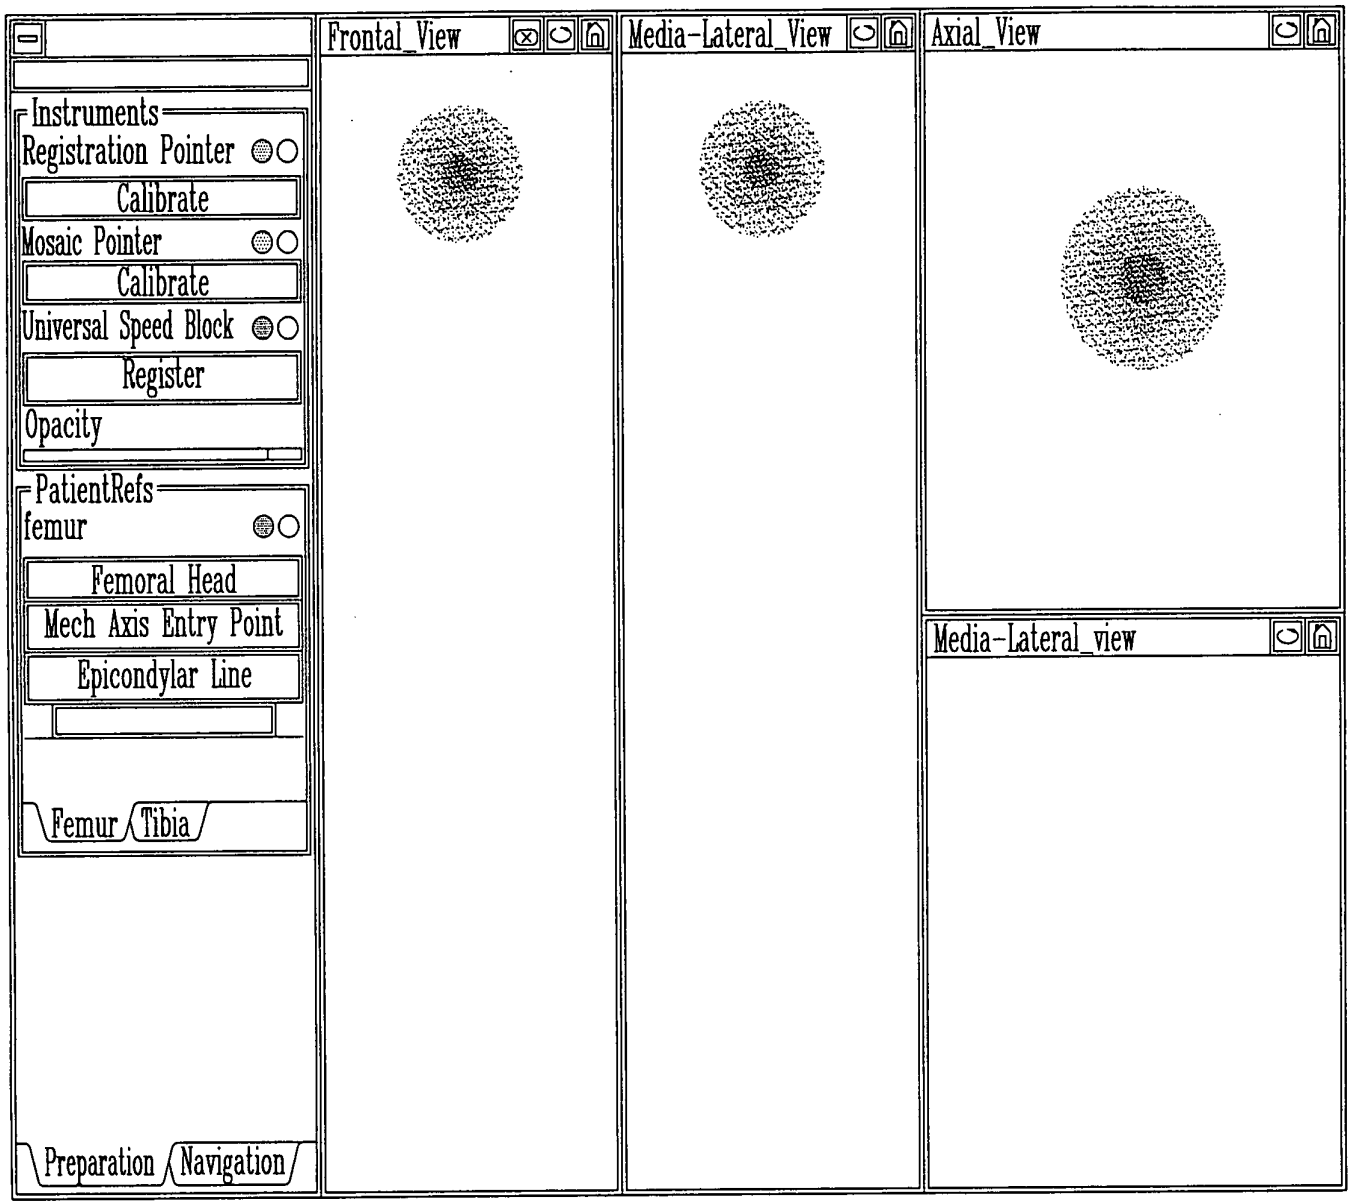
Instruments
Registration Pointer
Calibrate
Mosaic Pointer
Calibrate
Universal Speed Block
Register
Opacity
PatientRefs
femur
Femoral Head
Mech Axis Entry Point
Epicondylar Line
Femur
Tibia
Preparation
Navigation
Frontal_View
Media-Lateral_View
Axial_View
Media-Lateral_view

FIG_2

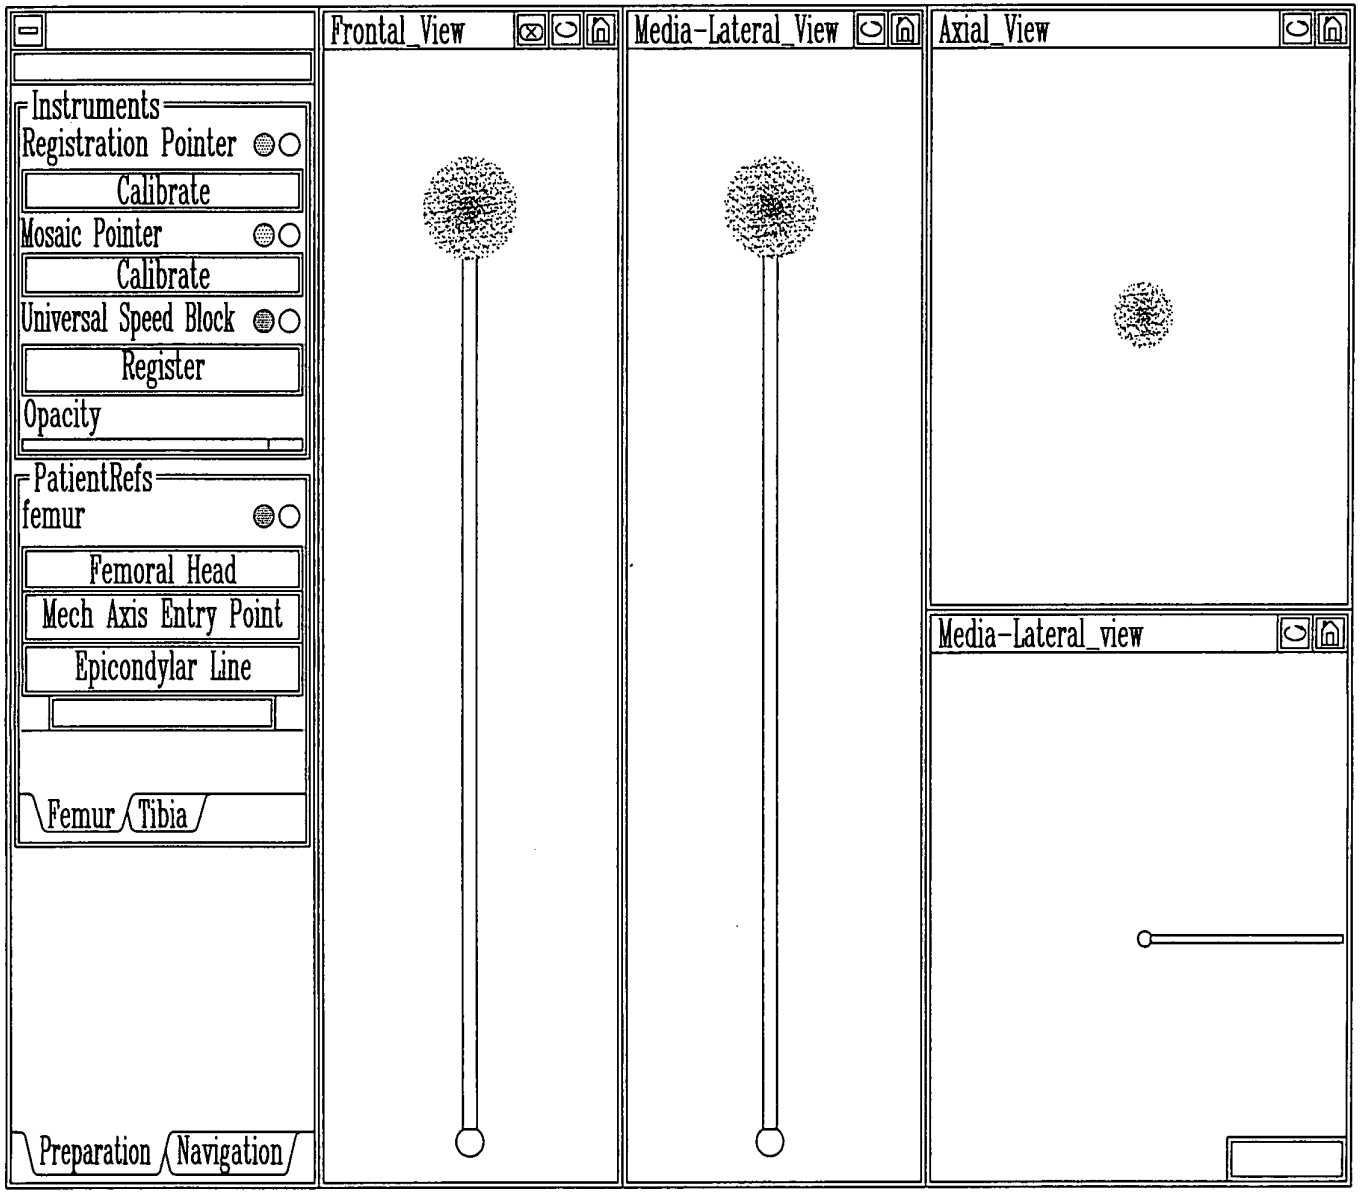
Instruments
Registration Pointer
Calibrate
Mosaic Pointer
Calibrate
Universal Speed Block
Register
Opacity
PatientRefs
femur
Femoral Head
Mech Axis Entry Point
Epicondylar Line
Femur
Tibia
Preparation
Navigation
Frontal_View
Media-Lateral_View
Axial_View
Media-Lateral_view

Fig. 3

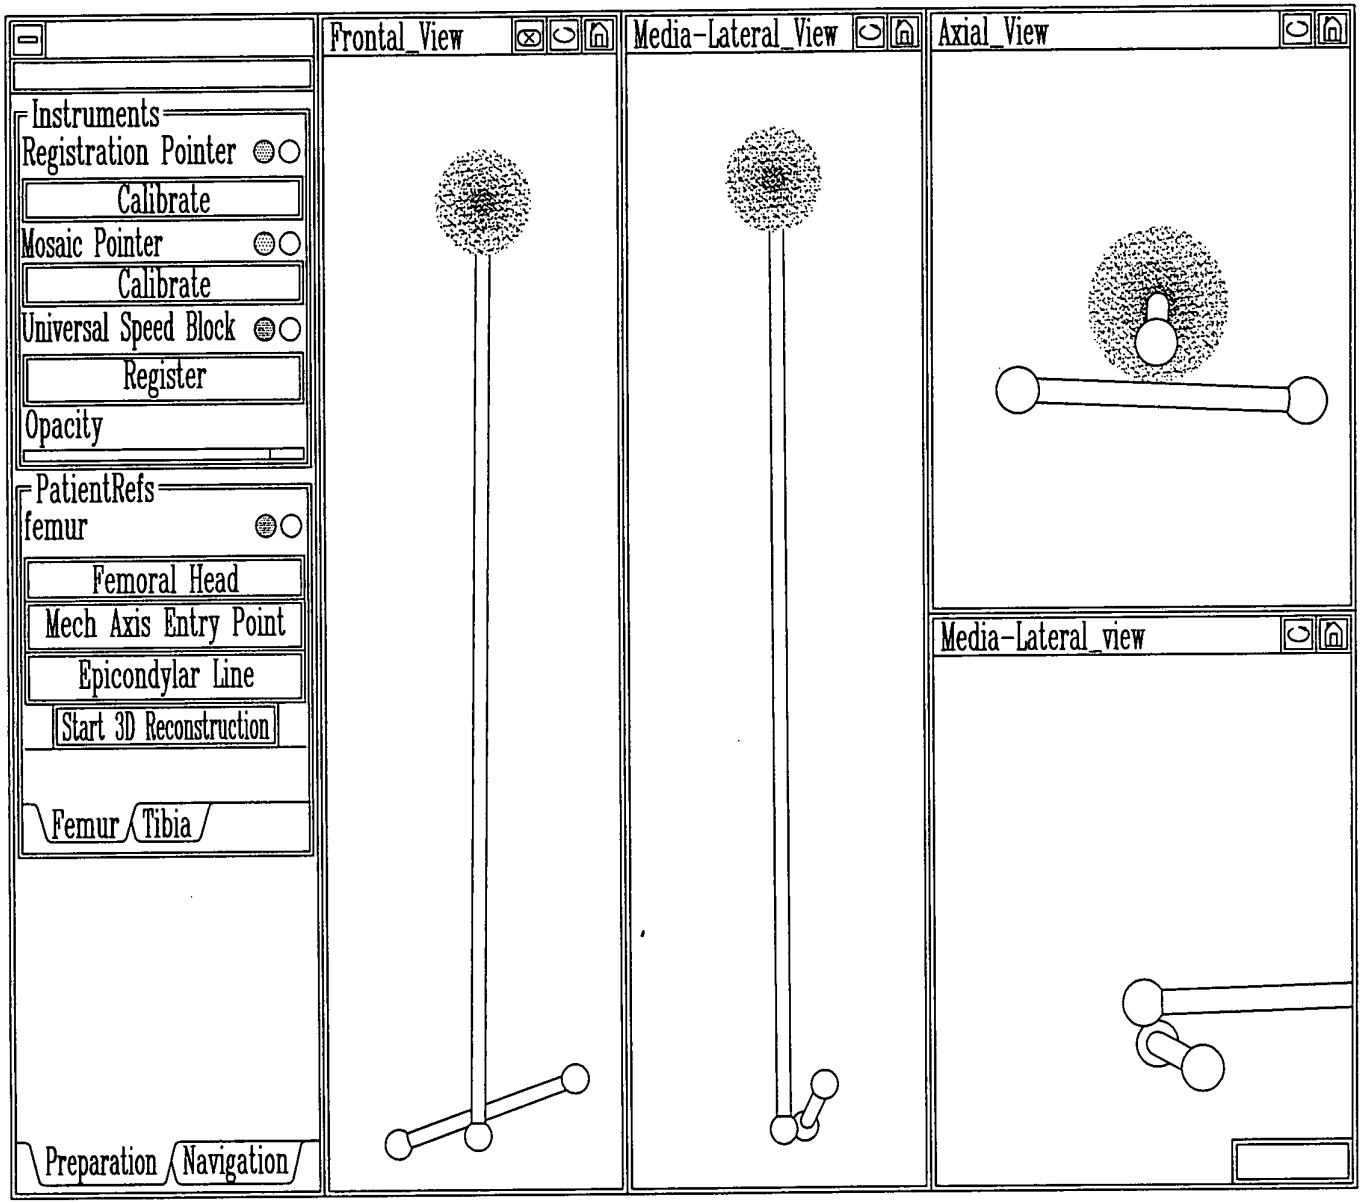
Instruments
Registration Pointer
Calibrate
Mosaic Pointer
Calibrate
Universal Speed Block
Register
Opacity
PatientRefs
femur
Femoral Head
Mech Axis Entry Point
Epicondylar Line
Start 3D Reconstruction
Femur
Tibia
Preparation
Navigation
Frontal_View
Media-Lateral_View
Axial_View
Media-Lateral_view

FIG 4

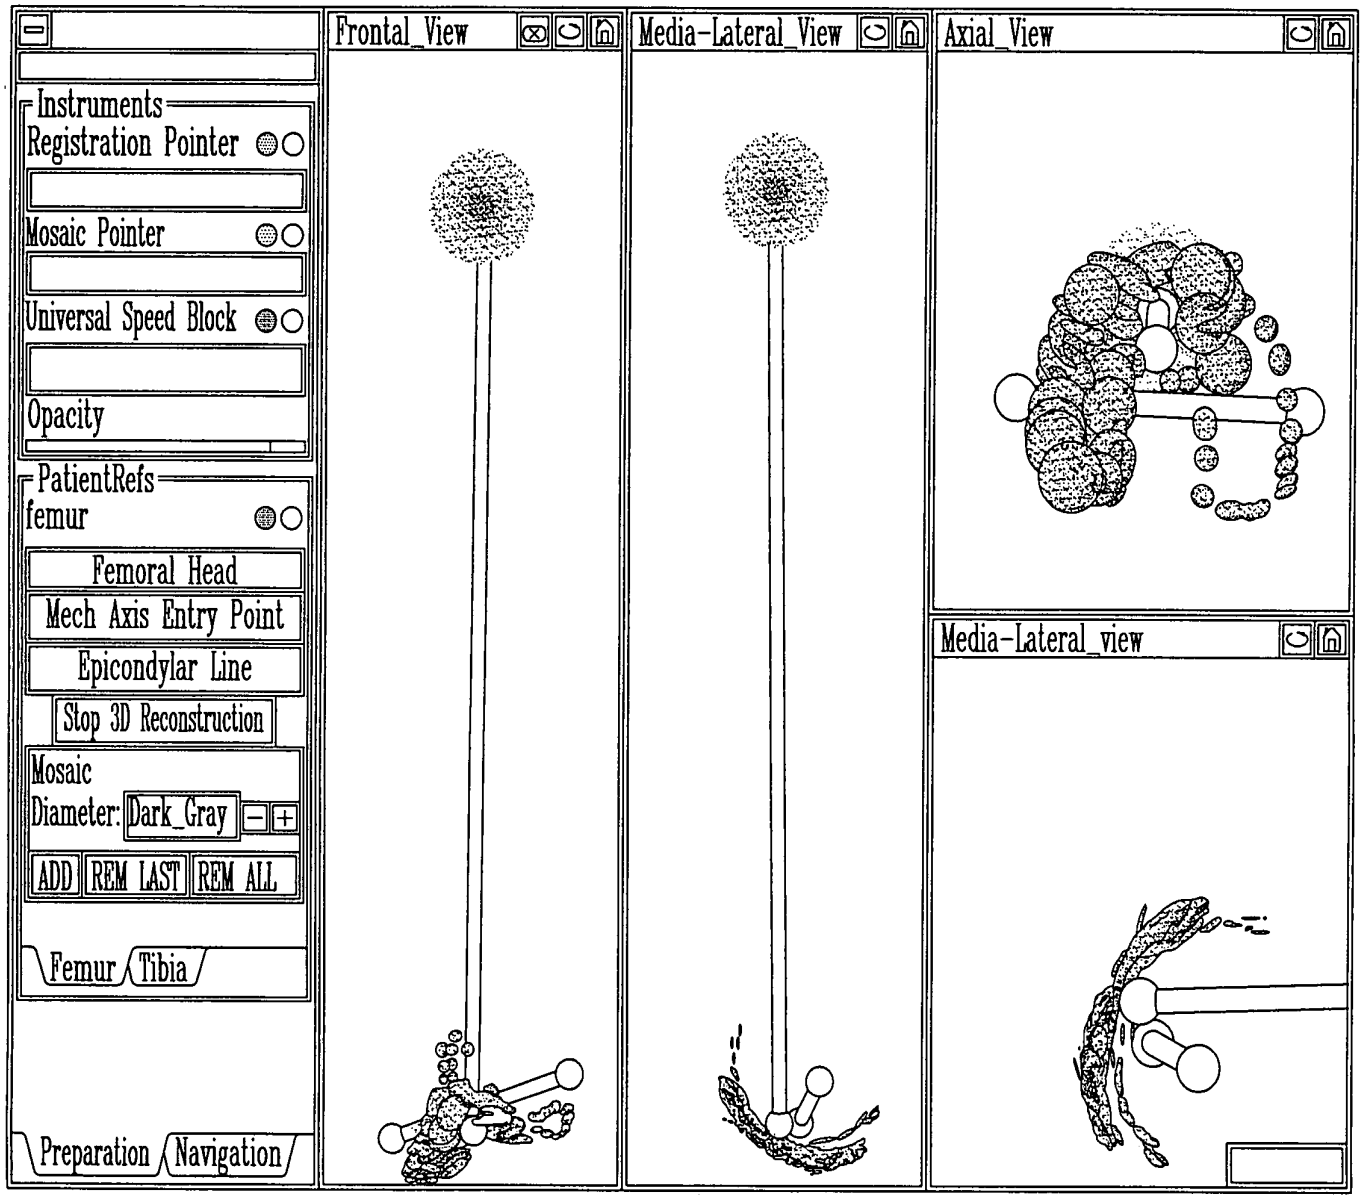
Instruments
Registration Pointer
Mosaic Pointer
Universal Speed Block
Opacity
PatientRefs
femur
Femoral Head
Mech Axis Entry Point
Epicondylar Line
Stop 3D Reconstruction
Mosaic
Diameter:
Dark_Gray
ADD
REM LAST
REM ALL
Femur
Tibia
Preparation
Navigation
Frontal_View
Media-Lateral_View
Axial_View
Media-Lateral_view

Fig. 5

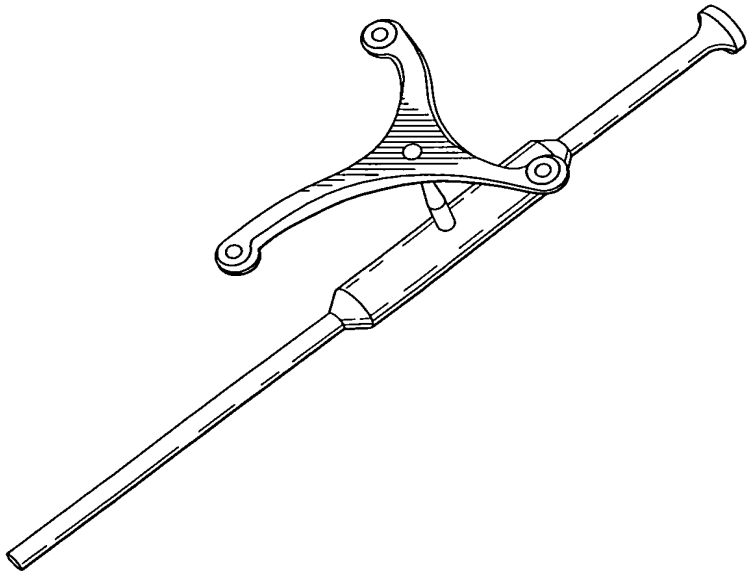

FIG 6